


MRI BREAST IMPLANTS - RUPTURE

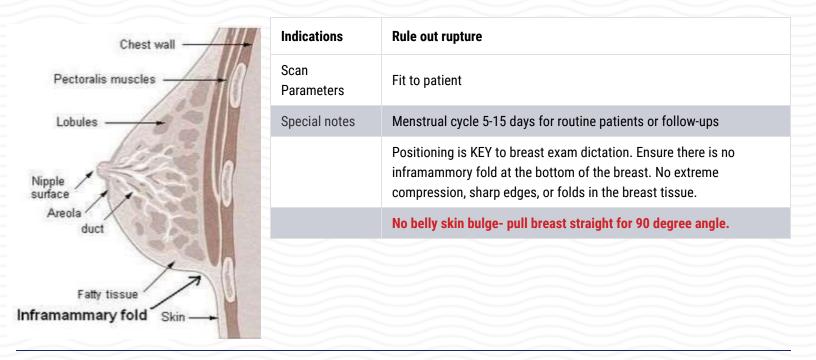

PLANE	Sequence	Fat Sat	Mode	SLT/SP	FOV	NS	GAP	NAQ	
Axial	STIR	No		4 mm	36 x 25	40	0.8	1	
Axial	Silicone sup			4 mm	36 x 25	40	0.8	1	
Axial	Saline sup			4 mm	34 x 26	79	0.8	1	
Axial	Saline/ FAT sup			4 mm	34 x 26	79	0.8	1	

Any deviation from protocol MUST be Radiologist approved. Rad Director will be notified if this occurs without prior approval.