


## MRI BREAST IMPLANTS DYNAMIC

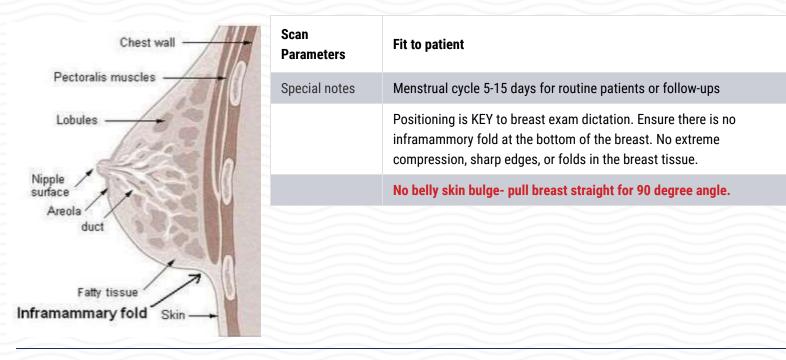

PLANE	Sequence	Fat Sat	Mode	SLT/SP	FOV	NS	GAP	NAQ
Axial	Silicone sup			4 mm	36 x 25	40	0.8	1
Axial	Saline sup			4 mm	36 x 25	79	0.8	1
Axial	Pre DYNAMIC			2.4 mm	34 x 26	79		1
Axial	DYNAMIC			2.4 mm	34 x 26	79		1
Sagittal	HIRES			3 mm	25	83		1

Any deviation from protocol MUST be Radiologist approved. Rad Director will be notified if this occurs without prior approval.